

ANAUXI

DISPOSABLE MICROCATHETER



Disposable Microcatheter



1/6

Flexible Three-layer Structure

The microcatheter is composed of resin outer layer, metallic supporting layer, and PTFE inner layer. The distal section is applied by coiled Pt-W alloy, and the proximal section is applied by braided stainless steel mesh. The static pressure resistance could reach up to 600PSI (4137KPa).

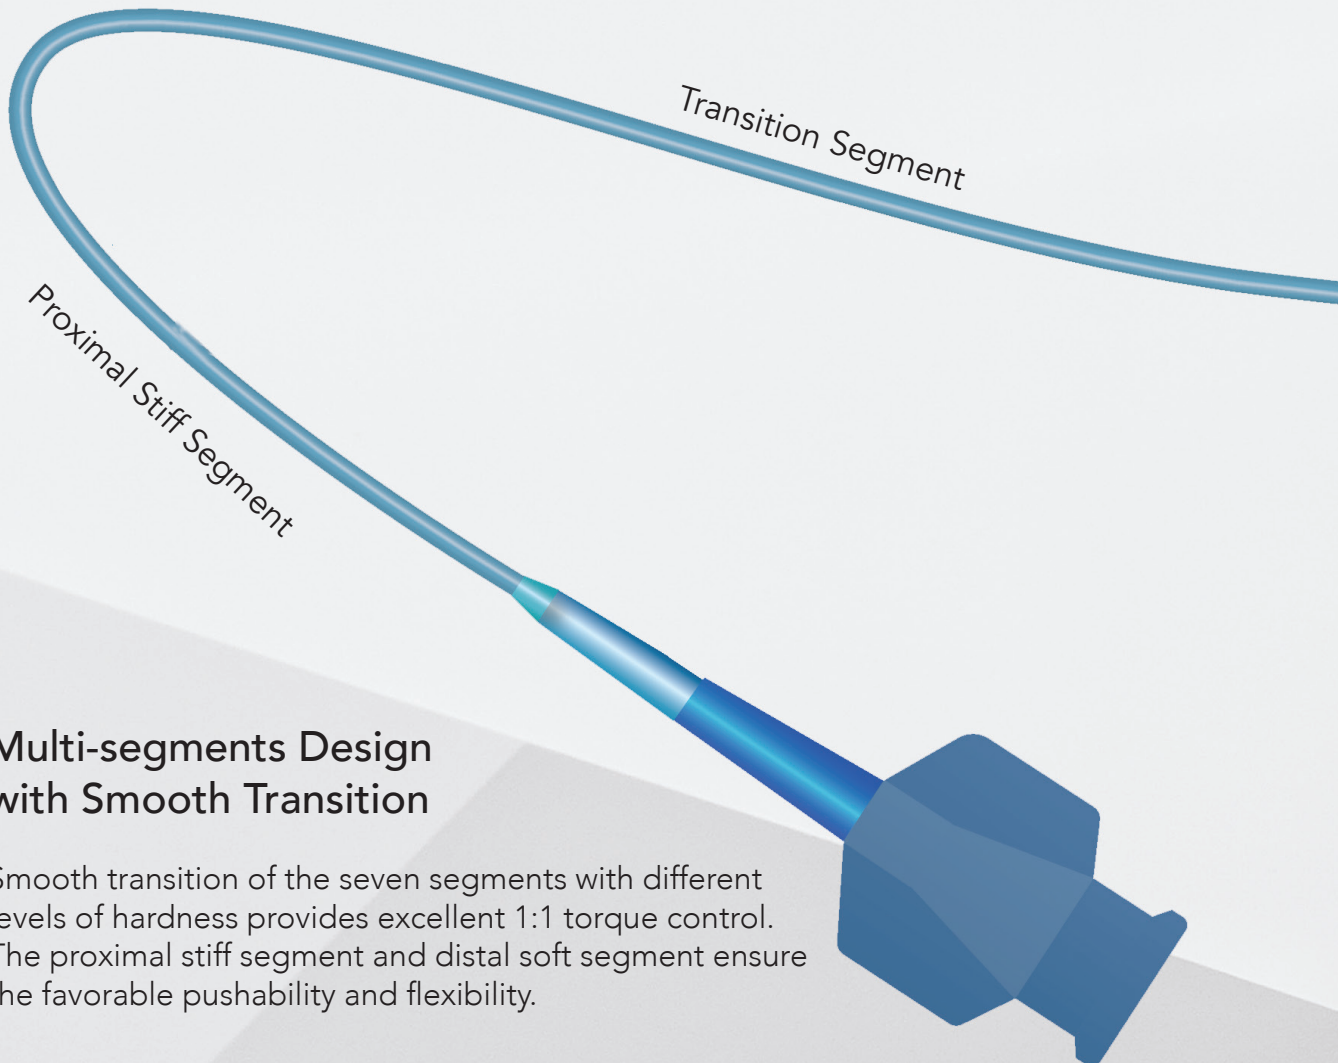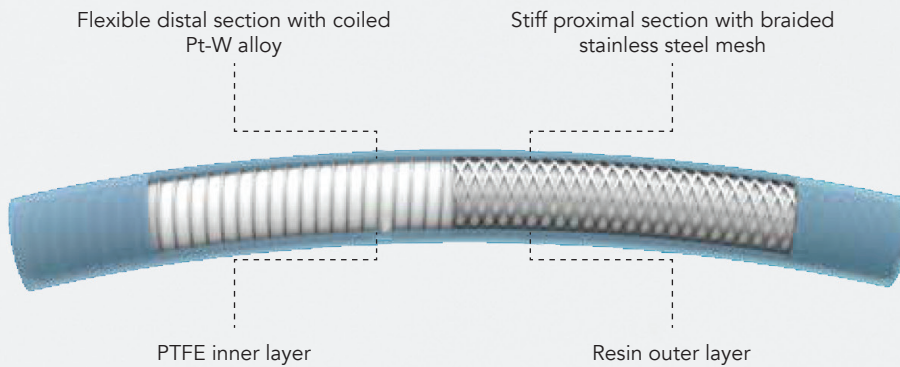

4/6


Multi-segments Design with Smooth Transition

Smooth transition of the seven segments with different levels of hardness provides excellent 1:1 torque control. The proximal stiff segment and distal soft segment ensure the favorable pushability and flexibility.

2/6

Excellent Supporting Performance

The distal soft segment is divided into two hardness levels, which could provide great supporting performance at aneurysm neck that help to prevent from the reactive force during the process of releasing the coil.

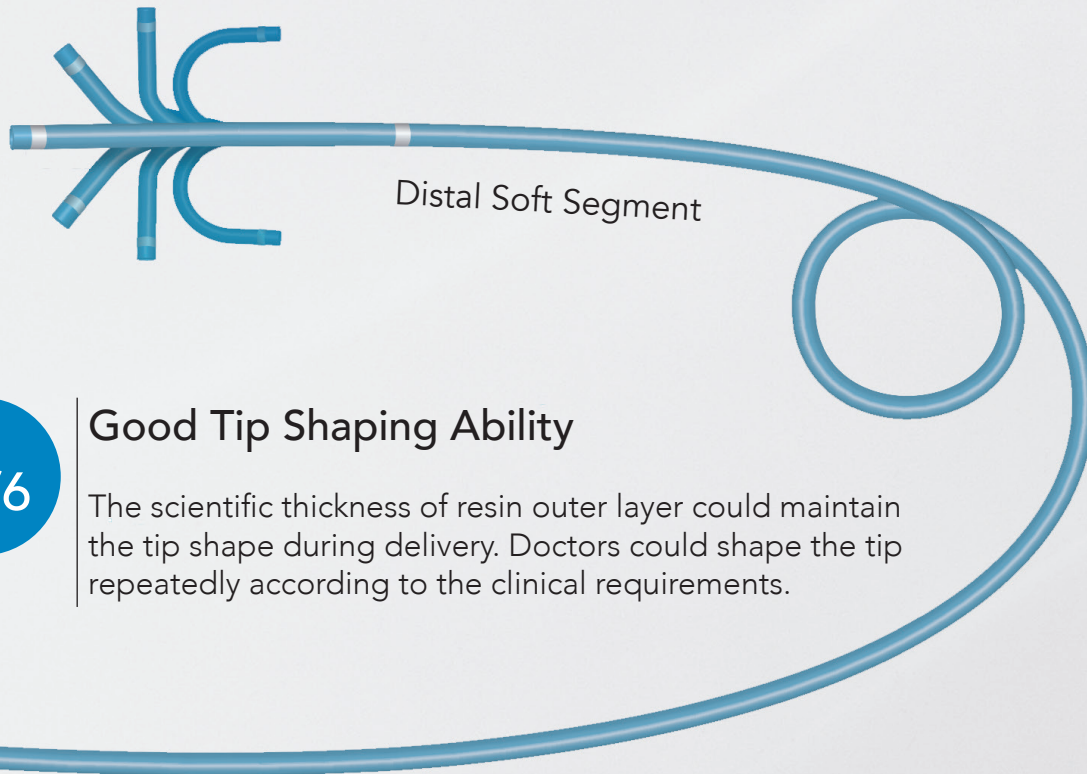

3/6

Good Tip Shaping Ability

The scientific thickness of resin outer layer could maintain the tip shape during delivery. Doctors could shape the tip repeatedly according to the clinical requirements.

5/6

Longer Distal Soft Segment

Longer distal soft segment enhances the crossability of the microcatheter in tortuous vessels, which makes it easy to manipulate.

6/6

Outstanding Distal Radiopacity

Other than the two markers, the whole soft segment also provides great radiopacity, which ensures the trackability of the microcatheter in the vessel.

ANAUXI

DISPOSABLE MICROCATETER

Disposable Microcatheter



Table Product Features of Anauxi™ Disposable Microcatheter

Specification	Effective Length	Soft Length	Proximal O.D.	Distal O.D.	Inner Diameter	Shape of distal tip	Marker
V-ANX-A10	150cm	50cm	2.2F/ 0.73mm	1.8F/ 0.60mm	0.015"	Straight	2Markers 3cm
V-ANX-A20	150cm	50cm	2.3F/ 0.76mm	1.9F/ 0.63mm	0.0165"	Straight	2Markers 3cm
V-ANX-A30	150cm	50cm	2.8F/ 0.93mm	2.3F/ 0.76mm	0.021"	Straight	2Markers 3cm
V-ANX-A40	140cm	30cm	2.8F/ 0.93mm	2.5F/ 0.83mm	0.027"	Straight	Single Marker



ANAUXI

DISPOSABLE MICROCATHETER

By



3403 NW 82nd Avenue, Suite 102 E.
Doral, Florida 33122
www.hosmed-inc.com